

# ASP Calibration Laboratory Traceability Chart

*Advantest Singapore Calibration Laboratory Traceability Chart*

**FOREIGN**

**SINGAPORE**

**National Standards Laboratories or Technology Institutes**

**A-STAR NMC**

**SAC-SINGLAS Accredited Laboratory OR Other Accredited Laboratory**

**DC/AC VOLTAGE  
DC/AC CURRENT  
RESISTANCE**  
FLUKE 5700A/EP  
FLUKE 5725A

**DIGITAL  
MULTIMETER**  
HP 3458A

**DC CALIBRATOR/  
SOURCE**  
KEITHLEY 263

**OPTICAL POWER  
METER/SENSORS**  
ADVANTEST  
TQ8210/Q82014/  
Q82017  
TQ8230/Q82311


**STANDARD  
RESISTANCE**  
ADVANTEST ASP-  
SR

**PRODUCT UNDER CALIBRATION ( Digital Multimeter, Electrometer, DC Voltage/Current Source, Optical Power meter/sensors )**

**DC / AC & Optical Power Standards**

# ASP Calibration Laboratory Traceability Chart

## *Advantest Singapore Calibration Laboratory Traceability Chart*

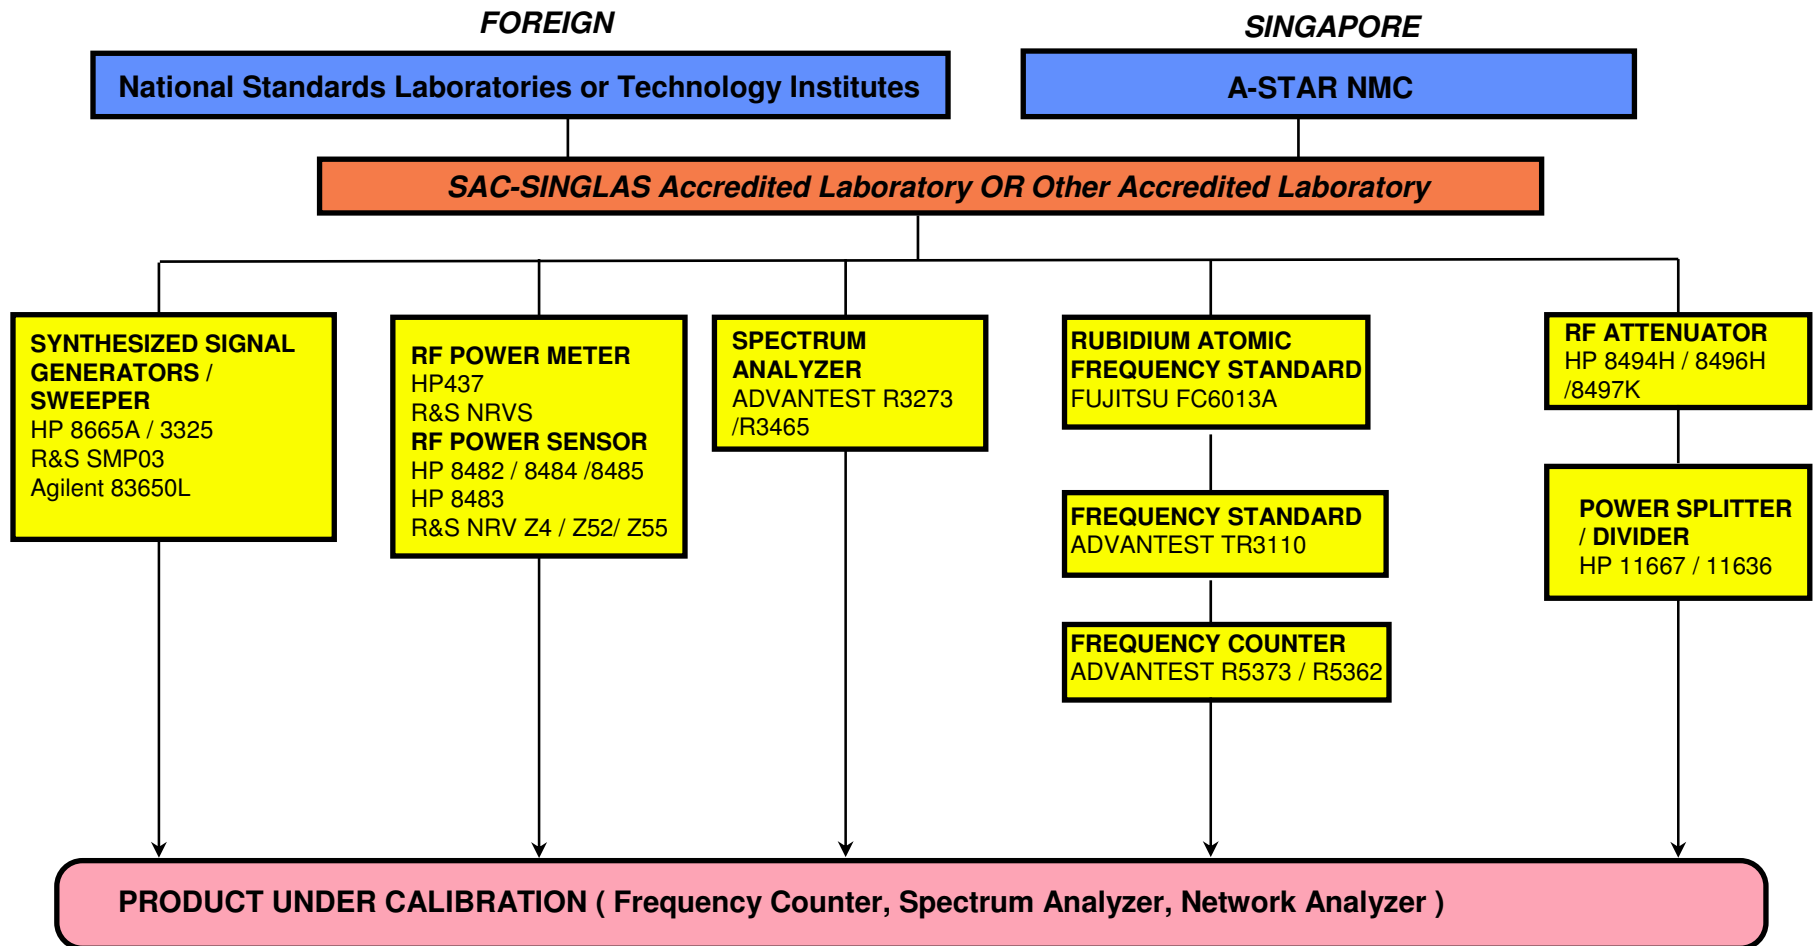

*Frequency / RF Power Standards*